

# Knobbe Martens Olson & Bear LLP

Intellectual Property Law

2040 Main Street  
Fourteenth Floor  
Irvine, CA 92614  
Tel 949-760-0404  
Fax 949-760-9502  
www.kmob.com



10/017916

Mark J. Kertz

September 29, 2005

Commissioner for Patents  
P.O. Box 1450  
Alexandria, VA 22313-1450

The PTO did not receive the following listed item(s)

Re: Title: DISTENDING PORTION FOR INTRAOCULAR LENS SYSTEM  
Letters Patent No. 6,764,511 B2  
Issued: July 20, 2004  
Our Reference: VGEN.004A

The PTO did not receive the following listed item(s) A check for \$100.00

Dear Sir:

Enclosed for filing is a Certificate of Correction in connection with the above-identified patent.

As the errors cited in the Certificate of Correction were incurred through no fault of the Patent Office, enclosed is our check in the amount of \$100. Please charge any additional fees to our Deposit Account No. 11-1410.

An explanation of the errors and the corrections is set forth below.

## First Error: Figures 18 and 39 of the Drawings

The application was originally filed with informal drawings. Due to an inadvertent error in the formal drawings that were later submitted, the formal drawings of Figures 18 and 39B did not match the informal drawings of Figures 18 and 39B as filed. The drawings of Figures 18 and 39B set forth in the enclosed Certificate of Correction properly match the drawings of Figures 18 and 39B as filed.

## Second Error: Specification Description of Figures 18 and 19

Figures 18 and 19 are described at Column 15, line 60 to Column 16, line 45. Figures 18 (as corrected) and 19 are depicted below:

10/04/2005 AKELECH1 00000033 111410 6764511

01 FC:1811 100.00 DA

San Diego  
619-235-8550

San Francisco  
415-954-4114


Los Angeles  
310-551-3450

Riverside  
951-781-9231


San Luis Obispo  
805-547-5580

OCT 11 2005

Certificate  
OCT 07 2005  
of Correction

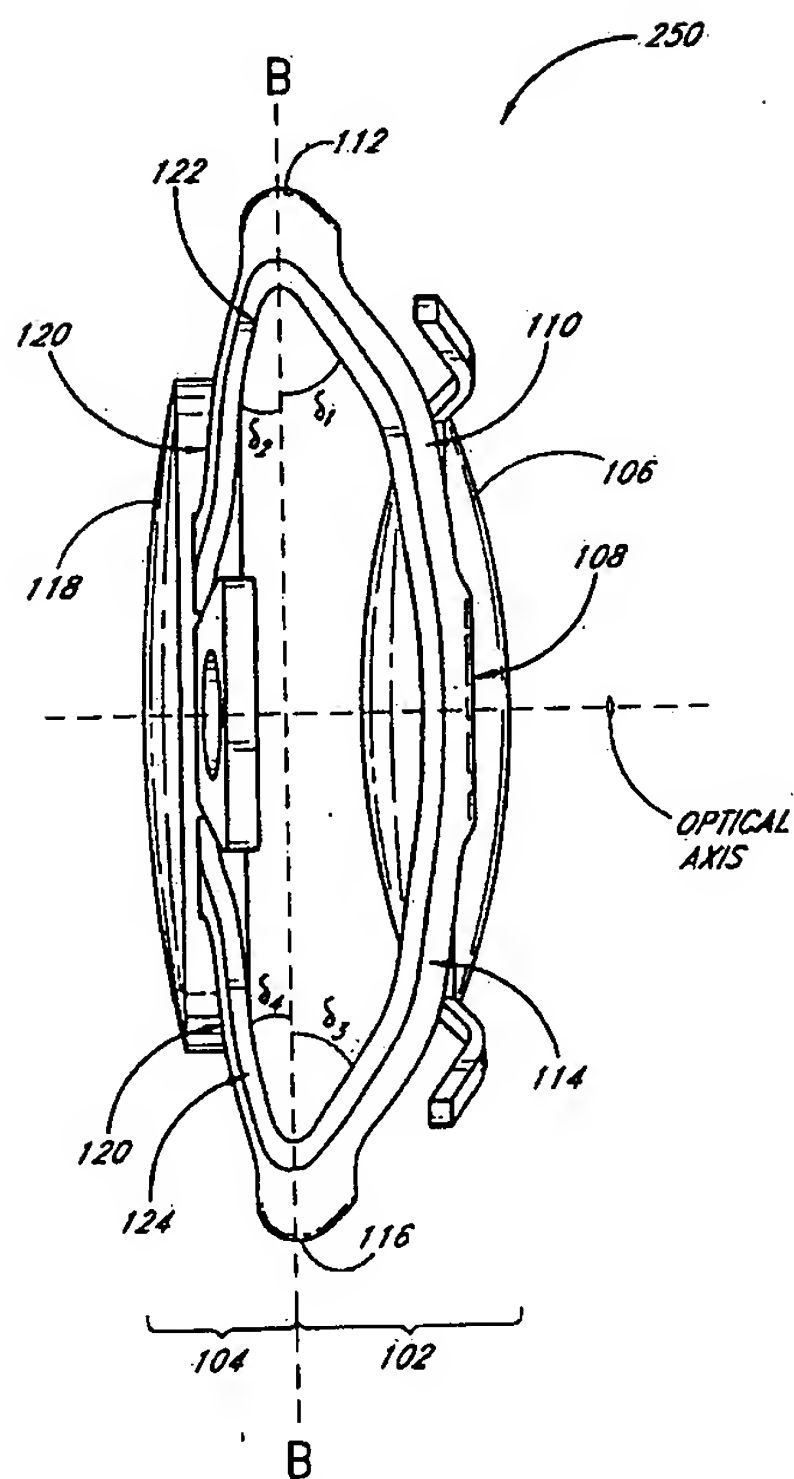

**FIG. 18**

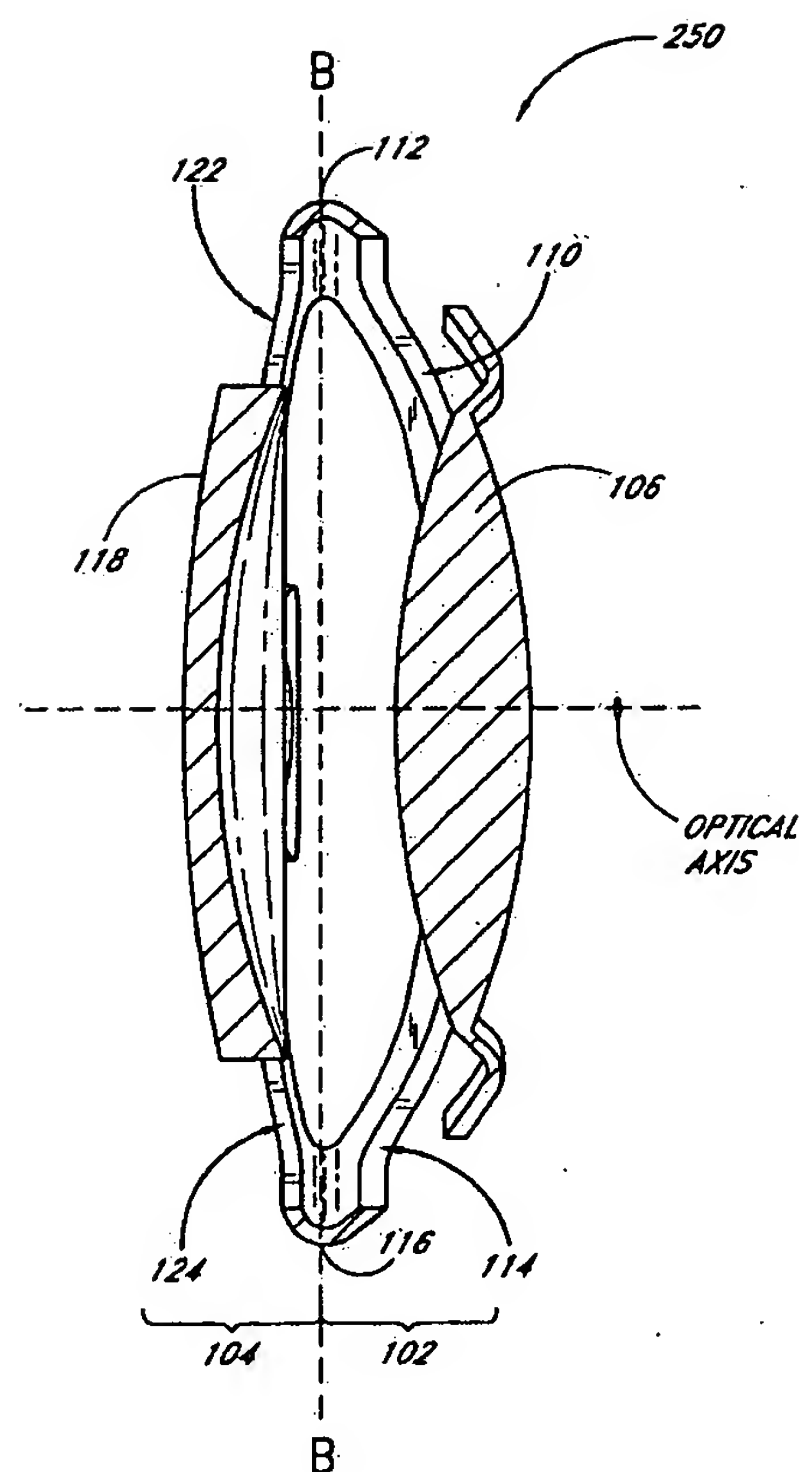

**FIG. 19**

The textual descriptions of Figures 18 and 19 contain a minor, obvious error at Column 16, line 10, in that the angles shown at the bottom of the lens system of Figures 18 and 19 are described as being substantially equal. Obviously, they are not. Indeed, the remainder of the description makes it abundantly clear that what is being described is a lens having asymmetry as viewed from the side, and that is exactly what the Figures depict. The correction to the

**Knobbe Martens Olson & Bear LLP**

Commissioner of Patents

September 29, 2005

Page -3-

specification made in the enclosed Certificate of Correction properly describes the angles as being unequal, and makes line 10 consistent with the other 52 lines of text that describe Figures 18 and 19, as well as with the figures themselves.

Respectfully submitted,

Knobbe, Martens, Olson & Bear, LLP

*Mark J. Kertz*

Mark J. Kertz

Registration No. 43,711

Customer No. 20,995

Enclosures

1894918:Cb 091505

OCT 11 2005

# UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

**PATENT NO. :** 6,764,511 *B2*


**DATED :** July 20, 2004

**INVENTOR(S):** Gholam Zadno-Azizi, et al.


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the specification, Col. 16, Line 10, delete "substantially equal" and substitute --unequal--.

In the drawings, change Figure 18 and Figure 39B to the following:

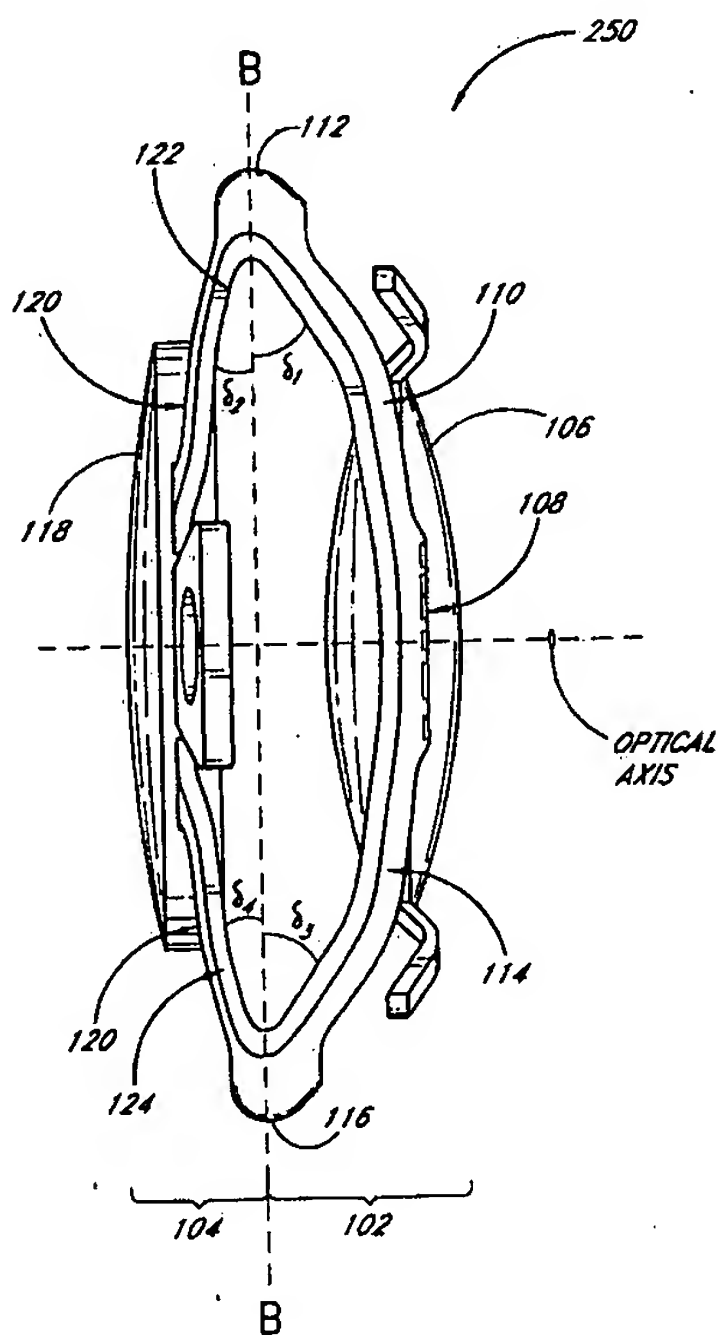

**FIG. 18**

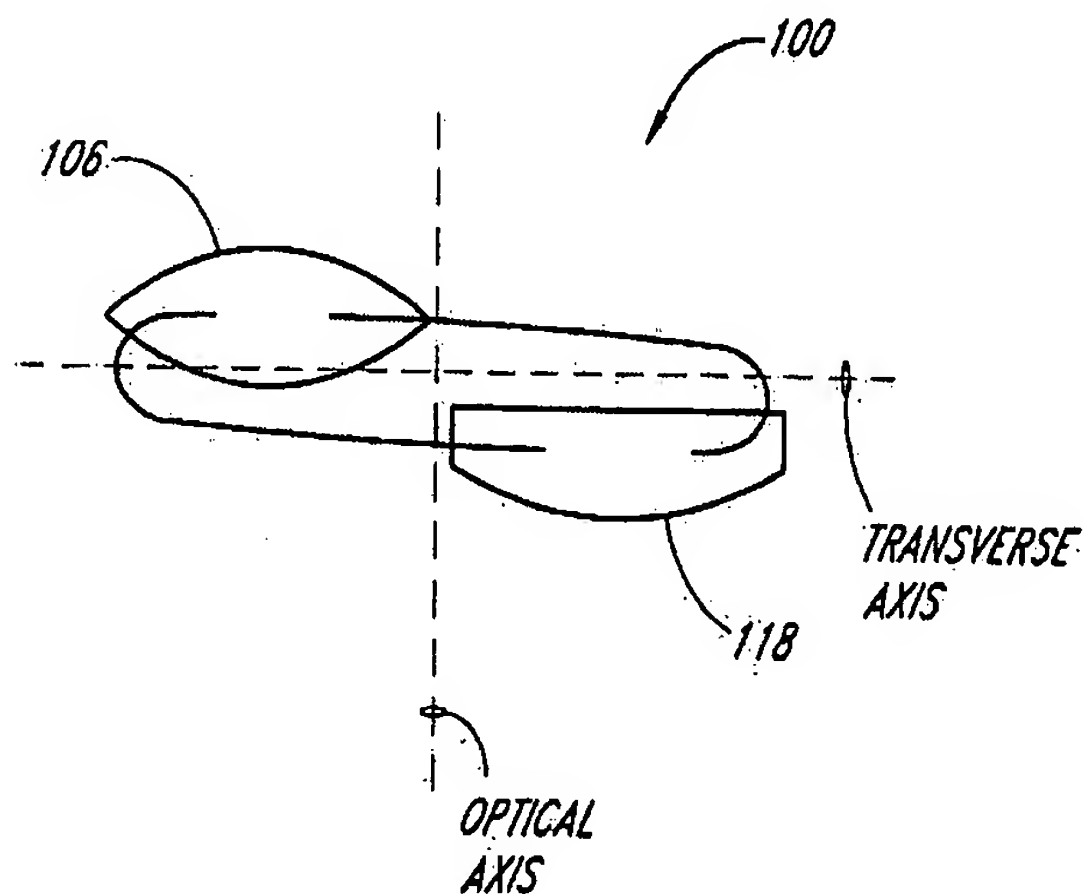

**FIG. 39B**

MAILING ADDRESS OF SENDER:

Mark J. Kertz  
KNOBBE, MARTENS, OLSON & BEAR, LLP  
2040 Main Street, 14<sup>th</sup> Floor  
Irvine, California 92614

PATENT NO. 6,764,511